


Sampling and recirculation facilities according to MEPC 60(33)



Ball valve on adjustment valve #27

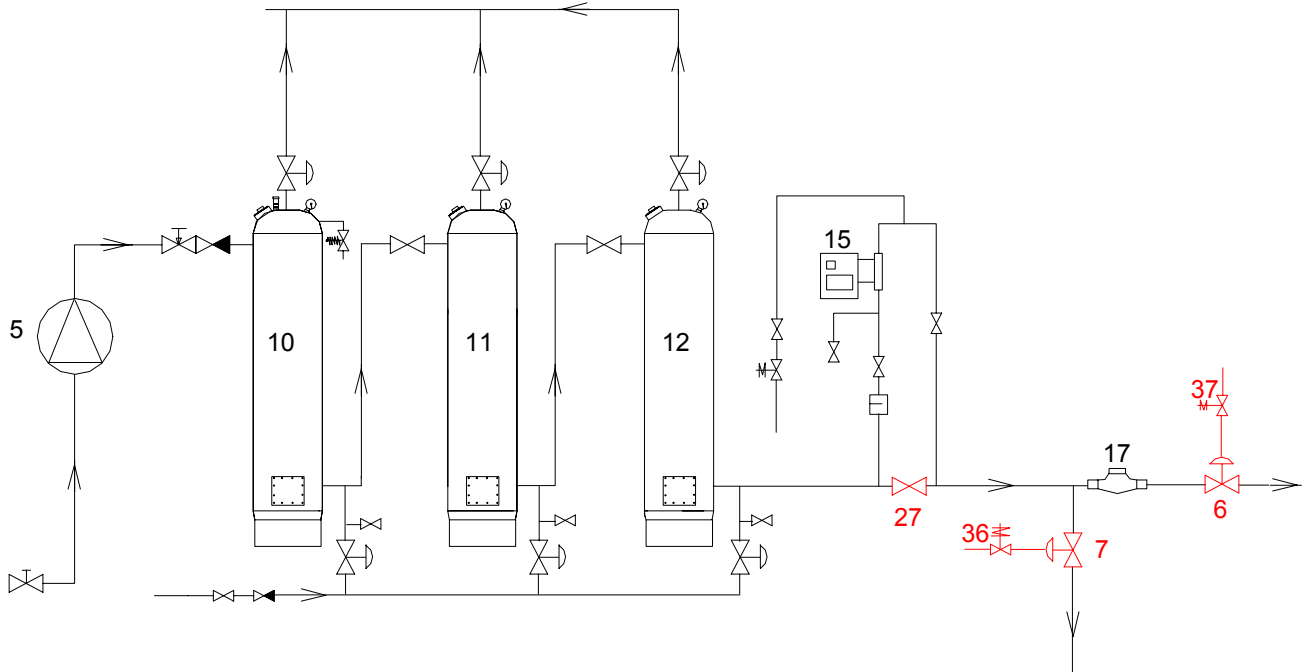

Pilot valve holder

